

BIO BS5

Handheld digital medical scope series

User's Manual



Wuxi Biomedical Technology Co.,Ltd

JIANG SU

1. General

BIO scope BS5 is a digital handheld scope used to record digital photographs and videos with different lens.

Otoscope lens: examine ear's canal and tympanic membrane

Rhinoscope lens: examine nasal cavity

Laryngoscope lens: examine throat


2. Scope

The medical scope is mainly used in hospital, Clinic and medical departments for doctors and nurses to examine ear, nasal and throat.

3. Components

The medical scope BS5 includes CMOS camera, fiber optic, LED bulb, 3 inches LCD screen, Rechargeable Battery, SD card , cables and suitable box.

Applicable camera lens: Otoscope, Rhinoscope, Laryngoscope

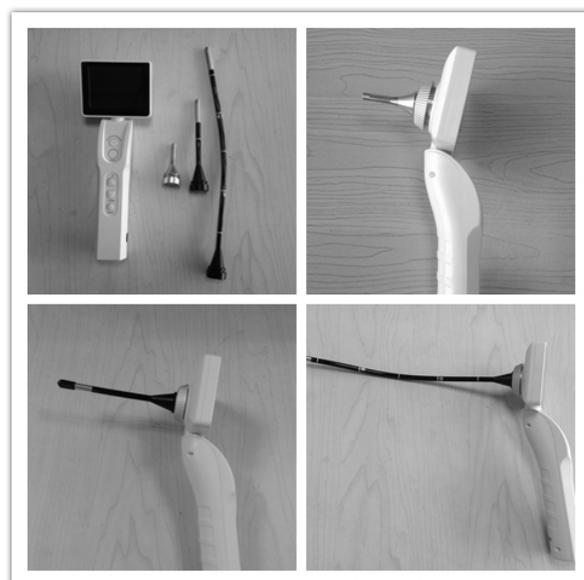

4. Specifications

Resolution: 720 x 480

Light source: Natural white (LED)

LCD screen: 3 inch high-definition LCD

Image format: JPEG, BMP

Media: Micro SD flash card

Power supply: rechargeable lithium battery

External power: 110~220 VAC, 50/60 Hz

Charging time: 5 hours

5. Operation Environment


Ambient temperature	10°C to +40°C
Relative humidity	≤ 80%
Atmospheric pressure	860hPa ~ 1060hPa

6. Storage Environment

Ambient temperature	-40°C to +55°C
Relative humidity range	10% to 100%, Including condensation
Atmospheric pressure	50KPa ~ 106KPa

7. Operating instructions

- Before operation, please make sure the appearance is not damaged or broken. If there are breaks in the device cover or other visual defects, please contact BIO service.
 - Take the lens and attach it on the handheld main unit. Rotate and fasten Lens in a clockwise direction.
 - Insert the SD card to the main unit.
 - Before the first use, connect USB connector to the power plug. Let the battery charged for fully charge.
- Note: Please pull the power plug before using, avoid using while charging.
- The user interface as following picture. Can be used to record digital photographs and videos. If want to delete the images and videos, select the format on the menu.

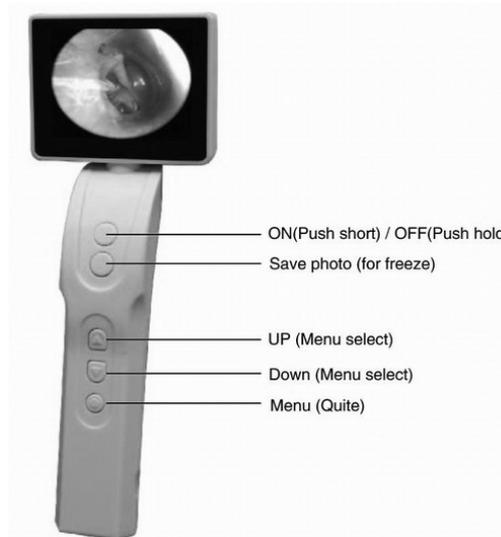

8. Troubleshooting

The possible causes of occurred errors and solving methods are listed below:

Errors	Possible Cause	Solutions
The scope is with fully charge, but not working.	The battery reaches lifetime or failure	contact the manufacturer or distributor to buy the spare battery.
The scope has power, but no image	CMOS damage, or circuit board fault	contact the manufacturer or distributor to repair
The freeze button or the other button not working	Button damage, or circuit board fault	contact the manufacturer or distributor to repair
The camera lens no light source	LED light source damage or circuit board fault	contact the manufacturer or distributor to repair

9. Cleaning and Disinfection

The BIO Scope is a precision photo electronic instrument that shall be cleaned and sterilized regularly. Please note following cleaning instructions:

- Power off the BIO Scope before cleaning it.
- Sterilize the handheld main unit with the soft cloth with 40% diluted alcohol.
- Clean the screen with soft cloth moistened with water. Do not use alcohol, diluents and detergent.

- Clean the lens before each use for a new patient:
Disinfect the lens with soft cloth or cotton ball moistened with alcohol (75% ethyl alcohol).

10. Notes and Warnings

- Do not place any objects on the scope, and don't let any liquid flow into the scope.
- To prevent fire or electrical shock, do not expose the scope to rain or moisture. Do not use the scope in flammable, explosive gas environment
- For the optional lens, avoid knocking, touching sharp objects and scratching. Or the images effect will be affected.
- When using otoscope lens, gently insert into the ear canal and have to keep a safety distance between the specula and tympanic membrane. Do not make the lens contact with ear's tympanic membrane.

11. Warranty

- The warranty of medical scope is 12 months since exportation date.
- Natural disasters, man-made damage, lack of reasonable care, disassembly, and warranty sticker had been torn up or phase-out parts are not included in the warranty.

Wuxi Biomedical Technology Co., Ltd.

Address: Room 408, No.801 Hongqiao road, Wuxi, Jiangsu, China

Zip code: 214072

Tel: 86-510-85572789

Fax: 86-510-85572789

Service Tel: 86-510-85572789

Http: <http://www.portable-ultrasound-scanner.com/>

E-mail : sales@cnbiomedical.com